

DECLARATION OF BLOOD PRESSURE MEASURING DEVICE EQUIVALENCE 2006

A SIGNED COPY WILL BE POSTED ON THE www.dableducational.org WEBSITE

SECTION A - Please complete all items online.

I Tomohiro Kukita Director of Omron Healthcare Europe B.V.
Name of a Company Director Company name

hereby state that there are no differences that will affect blood pressure measuring accuracy between the

Omron M3 (HEM-7200-E2)

Blood pressure measuring device for which validation is claimed

blood pressure measuring device and the

Omron M3 Intellisense (HEM-7051-E)

Existing validated blood pressure measuring device

blood pressure measuring device, which has previously passed the International protocol, the results of which were published as follows

Asmar R, Khabouth J, Topouchian J, El Feghali R, Mattar J

Authors(s)

Validation of three automatic devices for self-measurement of blood pressure according

to the International Protocol: The Omron M3 Intellisense (HEM-7051-E),

the Omron M2 Compact (HEM 7102-E), and the Omron R3-I Plus (HEM 6022-E)

Title

Journal of Hypertension

Publication

2006;24(suppl 4):S278

Year Volume Pages

The only differences between the devices involve the following components:

(When a component is not relevant, both Yes and No should be left blank. Please provide details on any differences below.)

Part I	1	Algorithm for Oscillometric Measurements	Yes <input type="checkbox"/>	No <input checked="" type="checkbox"/>
	2	Algorithm for Auscultatory Measurements	Yes <input type="checkbox"/>	No <input type="checkbox"/>
	3	Artefact/Error Detection	Yes <input type="checkbox"/>	No <input checked="" type="checkbox"/>
	4	Microphone(s)	Yes <input type="checkbox"/>	No <input type="checkbox"/>
	5	Pressure Transducer	Yes <input checked="" type="checkbox"/>	No <input type="checkbox"/>
	6	Cuff or Bladder	Yes <input checked="" type="checkbox"/>	No <input type="checkbox"/>
	7	Inflation Mechanism	Yes <input type="checkbox"/>	No <input checked="" type="checkbox"/>
	8	Deflation Mechanism	Yes <input type="checkbox"/>	No <input checked="" type="checkbox"/>
Part II	9	Model Name or Number	Yes <input checked="" type="checkbox"/>	No <input type="checkbox"/>
	10	Casing	Yes <input checked="" type="checkbox"/>	No <input type="checkbox"/>
	11	Display	Yes <input checked="" type="checkbox"/>	No <input type="checkbox"/>
	12	Carrying/Mounting Facilities	Yes <input type="checkbox"/>	No <input type="checkbox"/>
	13	Software other than Algorithm	Yes <input checked="" type="checkbox"/>	No <input type="checkbox"/>
	14	Memory Capacity/Number of stored measurements	Yes <input checked="" type="checkbox"/>	No <input type="checkbox"/>
	15	Printing Facilities	Yes <input type="checkbox"/>	No <input type="checkbox"/>
	16	Communication Facilities	Yes <input type="checkbox"/>	No <input type="checkbox"/>
	17	Power Supply	Yes <input type="checkbox"/>	No <input checked="" type="checkbox"/>
	18	Other Facilities	Yes <input type="checkbox"/>	No <input checked="" type="checkbox"/>

Brief explanation of differences and further relevant details:

5) The pressure sensor is replaced to a piezo electric sensor (NPS) from a capacitive sensor (CPSU), but the accuracy of blood pressure measurement is equivalent between NPS and CPSU.

6) Outer cloth is changed, no change on the size, shape and material on bladder.

10) The up button and the down button are added.

11) The symbol for body motion, the symbol for cuff wrapping guide and the indicator for blood pressure level are added.

13) The function to detect body motion and the function to guide cuff wrapping are included.

14) **2 user and 60 memories for each user instead of 42 memories.**



SECTION B - Complete all items, bar signatures and seal, online and print. Sign and seal it then send the original along with manuals for both devices to our address below.

Signature of Director Tomohiro Kukita

Name Tomohiro Kukita

Date 9 May 2012.

Signature of Witness [Signature]

Name Minoru Yoshimura

Address Omron Healthcare Europe B.V., Scorpius 33, 2132 LR Hoofddorp, The Netherlands

Company Stamp/Seal

OMRON HEALTHCARE EUROPE BV

Scorpius 33



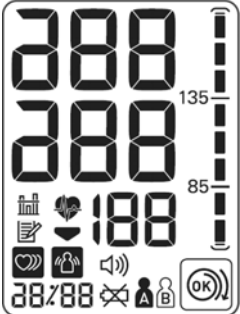

NL-2132 LR Hoofddorp

P.O.BOX 2050 NL-2130 GL Hoofddorp

TEL +31-23 5544700

FAX +31-23 5544701

Comparison of the Omron M3 (HEM-7200-E2) with the Omron M3 Intellisense (HEM-7051-E)

Devices	M3 (HEM-7200-E2)	M3 Intellisense (HEM-7051-E)
Pictures		
Display		
Validation		ESH-IP 2002
Device 1 Criteria	<p>Measurement</p> <p><i>Cuffs</i></p> <p>Universal (Arm circ. 22-42 cm) (Optional) ^{Note 2} 6</p> <p>Buttons/Switches</p> <p><i>Settings</i></p> <p>Up and down (Includes memory function) 10</p> <p><i>Measurement Records</i></p> <p>User ID 10</p> <p>Display/Symbols/Indicators</p> <p><i>Preparation</i></p> <p>Correct cuff wrapping indicator 11, 13</p> <p><i>Post Measurement</i></p> <p>Body movement error 3, 11, 13</p> <p><i>Measurement Records</i></p> <p>Memory recall number (Replaces pulse rate momentarily) 11</p>	

Devices	M3 (HEM-7200-E2)	M3 Intellisense (HEM-7051-E)
Device 1 Criteria (continued)	<p>Display/Symbols/Indicators (continued) <i>Measurement Records (continued)</i> User (A or B) 11</p> <p>Algorithms <i>Parameter Settings</i> Correct cuff wrapping detection 13</p> <p><i>Diagnostic</i> Body movement error detection 3, 13</p>	
Same Criteria	<p>Measurement <i>Accuracy</i> BP accuracy ± 3 mmHg 1, 5 Pulse accuracy ± 5% 1, 5</p> <p><i>Method</i> Oscillometric measurement method 1, 5 Pulse 40 bpm -180 bpm 1, 5 Measurements are from single inflations 13 Manually initiated measurements 13, 14</p> <p><i>Inflation</i> Inflation 0 mmHg - 299 mmHg 1, 5, 7 Automatic Inflation 7 Fuzzy Logic 7 Press button if BP > 220 mmHg 7 Manually adjustable inflation pressure 7</p> <p><i>Deflation</i> Automatic Deflation 8 Automatic safety release valve ^{Query 1, Note 3} 8</p> <p><i>Cuffs</i> Medium 146 mm × 446 mm (Arm circ. 22 to 32 cm) ^{Note 2} 6 Large (Arm circ. 32-42 cm) (Optional) ^{Note 2} 6</p> <p>Buttons/Switches <i>Power</i> On/Off with Start/Stop (O/I Start Label) 10</p> <p><i>Settings</i> Set 10</p> <p>Display/Symbols/Indicators <i>Measurement Procedure</i> Deflation symbol 11</p>	<p>Measurement <i>Accuracy</i> BP accuracy ± 3 mmHg 1, 5 Pulse accuracy ± 5% 1, 5</p> <p><i>Method</i> Oscillometric measurement method 1, 5 Pulse 40 bpm -180 bpm 1, 5 Measurements are from single inflations 13 Manually initiated measurements 13, 14</p> <p><i>Inflation</i> Inflation 0 mmHg - 299 mmHg 1, 5, 7 Automatic Inflation 7 Fuzzy Logic 7 Press button if BP > 220 mmHg 7 Manually adjustable inflation pressure 7</p> <p><i>Deflation</i> Automatic Deflation 8 Automatic safety release valve ^{Query 1, Note 3} 8</p> <p><i>Cuffs</i> Medium 146 mm × 446 mm (Arm circ. 22 to 32 cm) ^{Note 2} 6 Large (Arm circ. 32-42 cm) (Optional) ^{Note 2} 6</p> <p>Buttons/Switches <i>Power</i> On/Off with Start/Stop (O/I Start Label) 10</p> <p><i>Settings</i> Set 10</p> <p>Display/Symbols/Indicators <i>Measurement Procedure</i> Deflation symbol 11</p>

Devices	M3 (HEM-7200-E2)	M3 Intellisense (HEM-7051-E)
Same Criteria (continued)	<p>Display/Symbols/Indicators (continued) <i>Measurement Procedure (continued)</i></p> <p>Heartbeat symbol during deflation 11</p> <p>Audible pulse indicator during deflation (Optional) 18</p> <p>Beeps after measurement (Optional) 18</p> <p><i>Post Measurement</i></p> <p>SBP, DBP and Pulse 11</p> <p>Irregular heartbeat 11, 13</p> <p>Average symbol 11, 13</p> <p><i>Measurement Records</i></p> <p>Memory icon 11</p> <p><i>Date and Time</i></p> <p>Date and Time 11</p> <p>Date and Time (During memory recall) 11</p> <p><i>Power</i></p> <p>Low battery 11, 17</p> <p><i>Settings</i></p> <p>Audible pulse indicator mode active 11, 18</p> <p>Algorithms</p> <p><i>Averages</i></p> <p>Last 3 measurements (within 10 min of each other) mean 13</p> <p><i>Diagnostic</i></p> <p>Normotension/Hypertension 13</p> <p>135 / 85 mmHg thresholds 13</p> <p>Irregular heartbeat detection 13</p> <p>Case</p> <p><i>Display</i></p> <p>Single screen display 10</p> <p>Segment LCD 10</p> <p><i>Power</i></p> <p>4 "AA" batteries ~ 1500 measurements 17</p> <p>AC adapter (Optional) 17</p> <p>Automatic switch-off when not used for 5 min 17</p>	<p>Display/Symbols/Indicators (continued) <i>Measurement Procedure (continued)</i></p> <p>Heartbeat symbol during deflation 11</p> <p>Audible pulse indicator during deflation (Optional) 18</p> <p>Beeps after measurement (Optional) 18</p> <p><i>Post Measurement</i></p> <p>SBP, DBP and Pulse 11</p> <p>Irregular heartbeat 11, 13</p> <p>Average symbol 11, 13</p> <p><i>Measurement Records</i></p> <p>Memory icon 11</p> <p><i>Date and Time</i></p> <p>Date and Time 11</p> <p>Date and Time (During memory recall) 11</p> <p><i>Power</i></p> <p>Low battery 11, 17</p> <p><i>Settings</i></p> <p>Audible pulse indicator mode active 11, 18</p> <p>Algorithms</p> <p><i>Averages</i></p> <p>Last 3 measurements (within 10 min of each other) mean 13</p> <p><i>Diagnostic</i></p> <p>Normotension/Hypertension 13</p> <p>135 / 85 mmHg thresholds 13</p> <p>Irregular heartbeat detection 13</p> <p>Case</p> <p><i>Display</i></p> <p>Single screen display 10</p> <p>Segment LCD 10</p> <p><i>Power</i></p> <p>4 "AA" batteries ~ 1500 measurements 17</p> <p>AC adapter (Optional) 17</p> <p>Automatic switch-off when not used for 5 min 17</p>
Comparable Criteria	<p>Measurement <i>Measurement Records</i></p> <p>Memory: 60 measurements × 2 14</p>	<p>Measurement <i>Measurement Records</i></p> <p>Memory: 42 measurements 14</p>

Devices	M3 (HEM-7200-E2)	M3 Intellisense (HEM-7051-E)
Comparable Criteria (continued)	Measurement (continued) <i>Sensors</i> Pressure sensor: piezo-resistive ^{Note 1} 5	Measurement (continued) <i>Sensors</i> Pressure sensor: capacitive ^{Note 1} 5
	Display/Symbols/Indicators <i>Post Measurement</i> Measurement error $EE, E, E/E$ and E_r ^{Query 1, Note 4} 11 Hypertension (Indicator strip) 11, 13	Display/Symbols/Indicators <i>Post Measurement</i> Measurement error $EE, E, E/E$ and $E/\square 25$ ^{Query 1, Note 4} 11 Hypertension (Blinking heartbeat) 11, 13
Device 2 Criteria		Buttons/Switches <i>Measurement Records</i> Memory 10

Query	<p>Query There are differences in the descriptions of the rapid air release and error codes between the manuals. Similar queries were raised previously but it is not possible to infer scientifically that answers can be applied in these instances also. Can you confirm that the rapid air release is used in both devices and that the mapping of the errors, as described previously for specific devices also applies to these?</p> <table border="0" style="margin-left: auto; margin-right: auto;"> <thead> <tr> <th></th> <th>Rapid Air Release</th> <th>Error Codes²</th> </tr> </thead> <tbody> <tr> <td>M3 (HEM-7200-E2)</td> <td>No</td> <td>E EE E/E Er</td> </tr> <tr> <td>M3 Intellisense (HEM-7051-E)</td> <td>Yes¹</td> <td>E EE E/E E/oP</td> </tr> </tbody> </table> <p>Note 1 This is not included in the manual but stated in a previous communication. Note 2 From previous communications, the errors are equivalent and grouped as shown and <i>P</i> refers to a pressure level.</p> <p>Response We confirm that rapid air release function and fuzzy logic are applied for all devices. Regarding to the error codes, please refer the document which we sent previously. For equivalent models of M3 Intellisense, a group1 error codes apply but we change the device error code from “Eo25” to “Er” in order to avoid confusion form our customers. (“25” is not pressure).</p> <p>Comment The explanation is accepted</p>		Rapid Air Release	Error Codes ²	M3 (HEM-7200-E2)	No	E EE E/E Er	M3 Intellisense (HEM-7051-E)	Yes ¹	E EE E/E E/oP
	Rapid Air Release	Error Codes ²								
M3 (HEM-7200-E2)	No	E EE E/E Er								
M3 Intellisense (HEM-7051-E)	Yes ¹	E EE E/E E/oP								
Notes	<p>1 The Omron M3 (HEM-7200-E) was approved as equivalent to the Omron M3 Intellisense (HEM-7051-E) on 26/08/2010. The Omron M3 (HEM-7200-E2) is similar to the M3 (HEM-7200-E) device except that</p> <ul style="list-style-type: none"> a) The current pressure sensor (CPSU), a capacitive type, is changed to a new pressure sensor (NPS), a piezoelectric semiconductor type and b) The HEM-7200-E2 provides dual user facilities. <p>Details of comparatives tests between the sensors have been reviewed by dabl®Educational. Furthermore, the Omron M6 Comfort</p>									

		(HEM-7221-E8), which is the same as the Omron M6 Comfort (HEM-7221-E) except for a similar change in sensor, has been validated using the ESH-IP 2010 protocol and is recommended for use. Following a review of these documents, it was concluded that the change in sensor would not have a detrimental effect on the accuracy of the device.																		
	2	There is a change in the cloth used for the cuffs between those used for the Omron M3 (HEM-7200-E2) [CM2-9513256-6 Medium, CL2-9513255-8 Large and CW-9520534-2 Universal] and those used for the Omron M3 Intellisense (HEM-7051-E) [CM-4997086-7 & CM1-7935058-8 Medium and CL-4997065-4 Large]. The Omron M2 Basic (HEM-7116-E), approved for equivalence 26/08/2010 used CM2-9513256-6 & CM1-9997578-9 Medium and CL2-9513255-8 & CL1-9996760-3 Large.																		
	3	This note from the equivalence application for the HEM-7200-E is also applicable to the HEM-7200-E2.																		
		<i>The fact we have is that the group of M3 Intellisense (HEM-7051-E) have same deflation mechanism. They have same valves for deflation system, as you mentioned, which are the regular deflation valve (slow deflation during measurement) and the rapid exhaust valve (release pressure rapidly from air system in the device after measurement to make comfortable and safe patients). Also these 2 valves are operated by automatic. In some device's manual e.g. M3 Intellisense (HEM-7051-E), we mention only "Deflation: Automatic pressure release valve" as one function of automatic deflation so that we could provide easy explanation to end users.</i>																		
	4	This note from the equivalence application for the HEM-7200-E is also applicable to the HEM-7200-E2.																		
		<i>Regarding to Group1, when error appears in the device, the number in 2nd line indicates current air pressure. Therefore, EE and EE/0 indicates same error "cuff is under inflated" and also E and E/38 for measurement error. The number "0" and "38" means for "0mmHg" and "38mmHg". These are no more than example description for manual. However, in order not to confuse users, we are not using this description in manual any more. Regarding to Eo25 and Er25, these indicates same error "device error". These differences come from hardware limitation from LCD display. We consider these error codes have no difference and there is no algorithm change.</i>																		
	Group 1 Error Codes																			
	<table border="1" style="margin-left: auto; margin-right: auto;"> <thead> <tr> <th>Models</th> <th colspan="4">Error codes</th> <th>Ref</th> </tr> </thead> <tbody> <tr> <td>M3 Intellisense</td> <td>EE</td> <td>E</td> <td>E/E</td> <td>Eo25</td> <td>Z</td> </tr> <tr> <td>M3</td> <td>EE</td> <td>E/38</td> <td>E/E</td> <td>Er25</td> <td>Y</td> </tr> </tbody> </table>		Models	Error codes				Ref	M3 Intellisense	EE	E	E/E	Eo25	Z	M3	EE	E/38	E/E	Er25	Y
Models	Error codes				Ref															
M3 Intellisense	EE	E	E/E	Eo25	Z															
M3	EE	E/38	E/E	Er25	Y															
Recommendation	Equivalence is recommended.																			
Date	02/07/2012																			